



**World Calibration Centre
for Aerosol Physics**

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig



**Leibniz Institute for
Tropospheric Research**

CPC Model: TSI CPC 3750

CPC Serial Number: 3750194201

Customer: TSI Instruments Ltd.

Description: Calibration of a Condensation Particle Counter (CPC, Model 3750)

Date of Calibration: November 13, 2019

Summary of Intercomparison:

The candidate passed the quality standards of ACTRIS and GAW. The candidate reached 99% efficiency at 40 nm. The Dp50 is at 6.60 nm. The CPC efficiency curve corresponds to the standard of ACTRIS and GAW.

Certificate / Reference: WCCAP

Date of issue: November 13, 2019 Signature:

Reviewed by: **TROPOS** Name: **Kay Weinhold**

Page 1 / 4



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

Date of arrival of instrument in calibration lab:

November 11, 2019

Instrument:

Condensation Particle Counter

Model and serial number of instrument:

CPC 3750 S/N 3750194201

Result of physical inspection:

no damages

Result of functional test:

functional test successful, no problems

Internal parameters of instrument

nominal flow rate 1.0 l/min

**Model and identification number of
aerosol electrometer:**

TSI Electrometer Model 3068, S/N 70838596

Electrometer calibration certificate:

*September 5, 2018, calibrated at PTB
Braunschweig*

**Corrections of electrometer, for instance,
differing flow rate:**

*Within tolerance range (+/-2%); reference: 4.0
l/min, measured: 4.000 l/min*

Software for recording:

*LabView 2010; National Instruments; Program
„LabCount.vi“*

Date of calibration:

November 13, 2019

Lab temperature and pressure:

24.5°C, 982.5 mbar

Measured aerosol flow rate of CPC:

1.009 l/min

Uncertainty in measured flow rate:

3%

Flowmeter used:

*Gilian Gilibrator V; S/N 1711008-S,
January, 2018*

Particles and gases used for calibration:

silver particles and nitrogen

Method of particle generation:

tube furnace generator

Zero measurement of instrument:

0 particles/cm³ in 5 minutes

Results (using pulse output):

Particle size (nm)	40	30	20	15	10
Number concentration (cm ⁻³)	1271	1263	1496	1255	1261
Counting efficiency η	0.98	0.99	0.99	0.99	0.88
Particle size (nm)	09	08	07	06	
Number concentration (cm ⁻³)	1344	856	799	500	
Counting efficiency η	0.81	0.71	0.56	0.36	



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

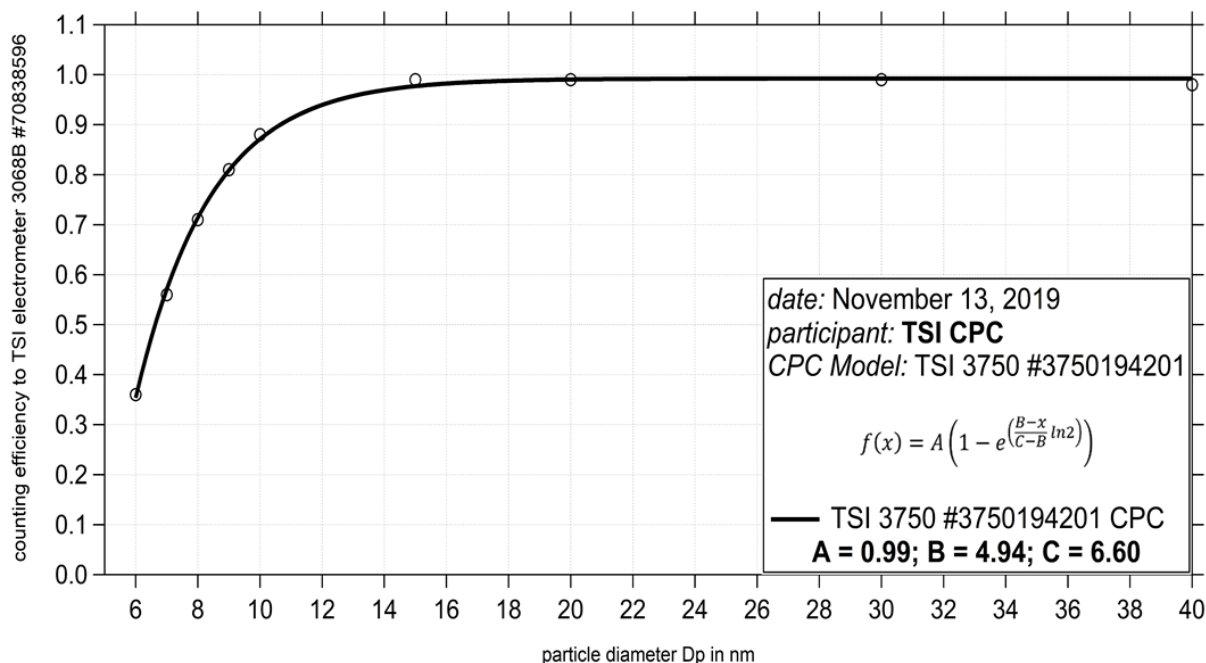


Fig. 1: Counting efficiency for CPC 3750 S/N 3750194201 against aerosol electrometer 3068 S/N 70838596; silver particles between 6 and 40 nm were used for calibration; the calculated D_{p50} is 6.60 nm.

Status information:

Status	<i>T SAT</i>	<i>T CON</i>	<i>T OPT</i>	<i>T CAB</i>	<i>P AMB</i>	<i>P VAC</i>
from display	39.0	18.0	40.0	24.5	98.9	80.9
Status	<i>P OR</i>	<i>P NO</i>	<i>Laser</i>	<i>LV</i>	<i>flow</i>	<i>P INLET</i>
from display	77.1	2.49	37	full	1.009	-0.4

Results (using pulse output):

without coincidence correction					
Concentration EM in #/cm ³	66849	58164	50013	43197	32294
Number concentration without coincidence correction (cm-3)	52992	47123	41178	36197	27900
Counting efficiency η	0.79	0.81	0.82	0.83	0.86
Concentration EM in #/cm ³	19887	11244	5127	1177	
Number concentration without coincidence correction (cm-3)	17854	10428	4901	1148	
Counting efficiency η	0.89	0.92	0.95	0.97	



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

with coincidence correction					
Concentration EM in $\#/cm^3$	66849	58164	50013	43197	32294
Number concentration with coincidence correction (cm^{-3})	68640	59396	50475	43417	32191
Counting efficiency η	1.02	1.02	1.00	1.00	0.99
Concentration EM in $\#/cm^3$	19887	11244	5127	1177	
Number concentration with coincidence correction (cm^{-3})	19721	11247	5216	1245	
Counting efficiency η	0.99	1.00	1.01	1.05	

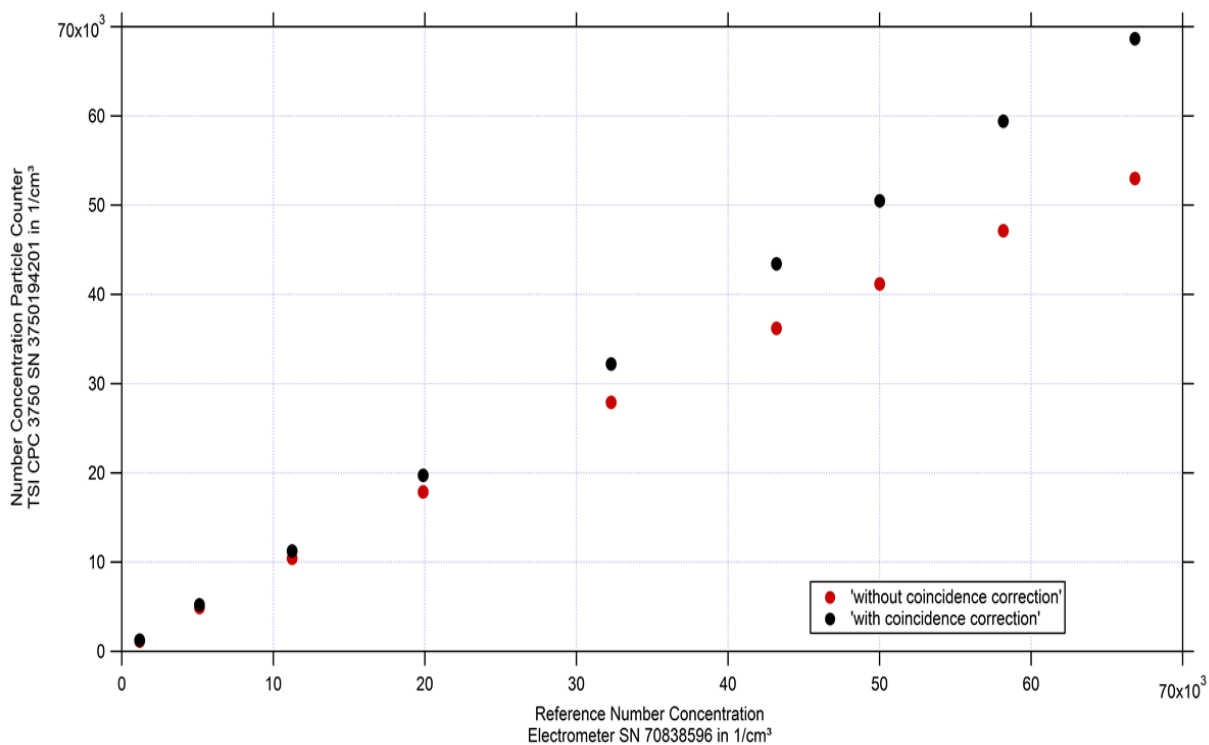


Fig. 2: Linearity test for TSI CPC 3750 SN 3750194201 against aerosol electrometer 3068 SN 70838596; silver particles with a diameter of 30 nm were used for number concentrations between 1000 and 70000 particles per cm^3 .

Date of issue: November 13, 2019

Reference: TSI electrometer, model 3068, SN 70838596

Reviewed: TROPOS / Kay Weinhold

Page 4 / 4