



Leibniz Institute for  
Tropospheric Research

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig

## Intercomparison of Condensation Particle Counter

*Project No.:* CPC-2019-5-4

*Principal Investigator:* Prof. Jean-François Doussin

*Home Institution:* FORTH, Greece

*Participant:* Jack Kodros and Christos Kaltsonoudis  
*Candidate:* FORTH UCPC  
*Counter (SN):* TSI CPC Model 3775 #71046188

*Location of the quality assurance:* TROPOS Leipzig, lab 130

*Comparison period:* October 08, 2019

*Last Intercomparison (with Project No.):*

*TROPOS Reference Instrument:* Electrometer: TSI model 3068B  
#70838596, Last calibration in September 2018

*Additional Equipment:* Bubble flow meter 'Gilibrator', Gilian (Sensidyne)  
#1711008-S, Last calibration in January 2018

### Summary of Intercomparison

*Status:*

The candidate passed the quality standards of ACTRIS and GAW. The candidate reached 98% efficiency at 40 nm. The Dp50 is at 3.35 nm. The CPC efficiency curve corresponds to the standard of ACTRIS and GAW.

Page 1 / 4


Leibniz-Institut für Troposphärenforschung e.V.  
Telefon: +49 341 2717-7060  
Telefax: +49 341 2717-99-7060  
info@tropos.de  
<http://www.tropos.de>

Commerzbank Leipzig  
KTO 102 14 50  
BLZ 860 400 00  
IBAN: DE77 8604 0000 0102 1450 00  
SWIFT CODE: COBADEFF 860

Mitglied der  
  
Leibniz-Gemeinschaft

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig

### Laboratory Setup:

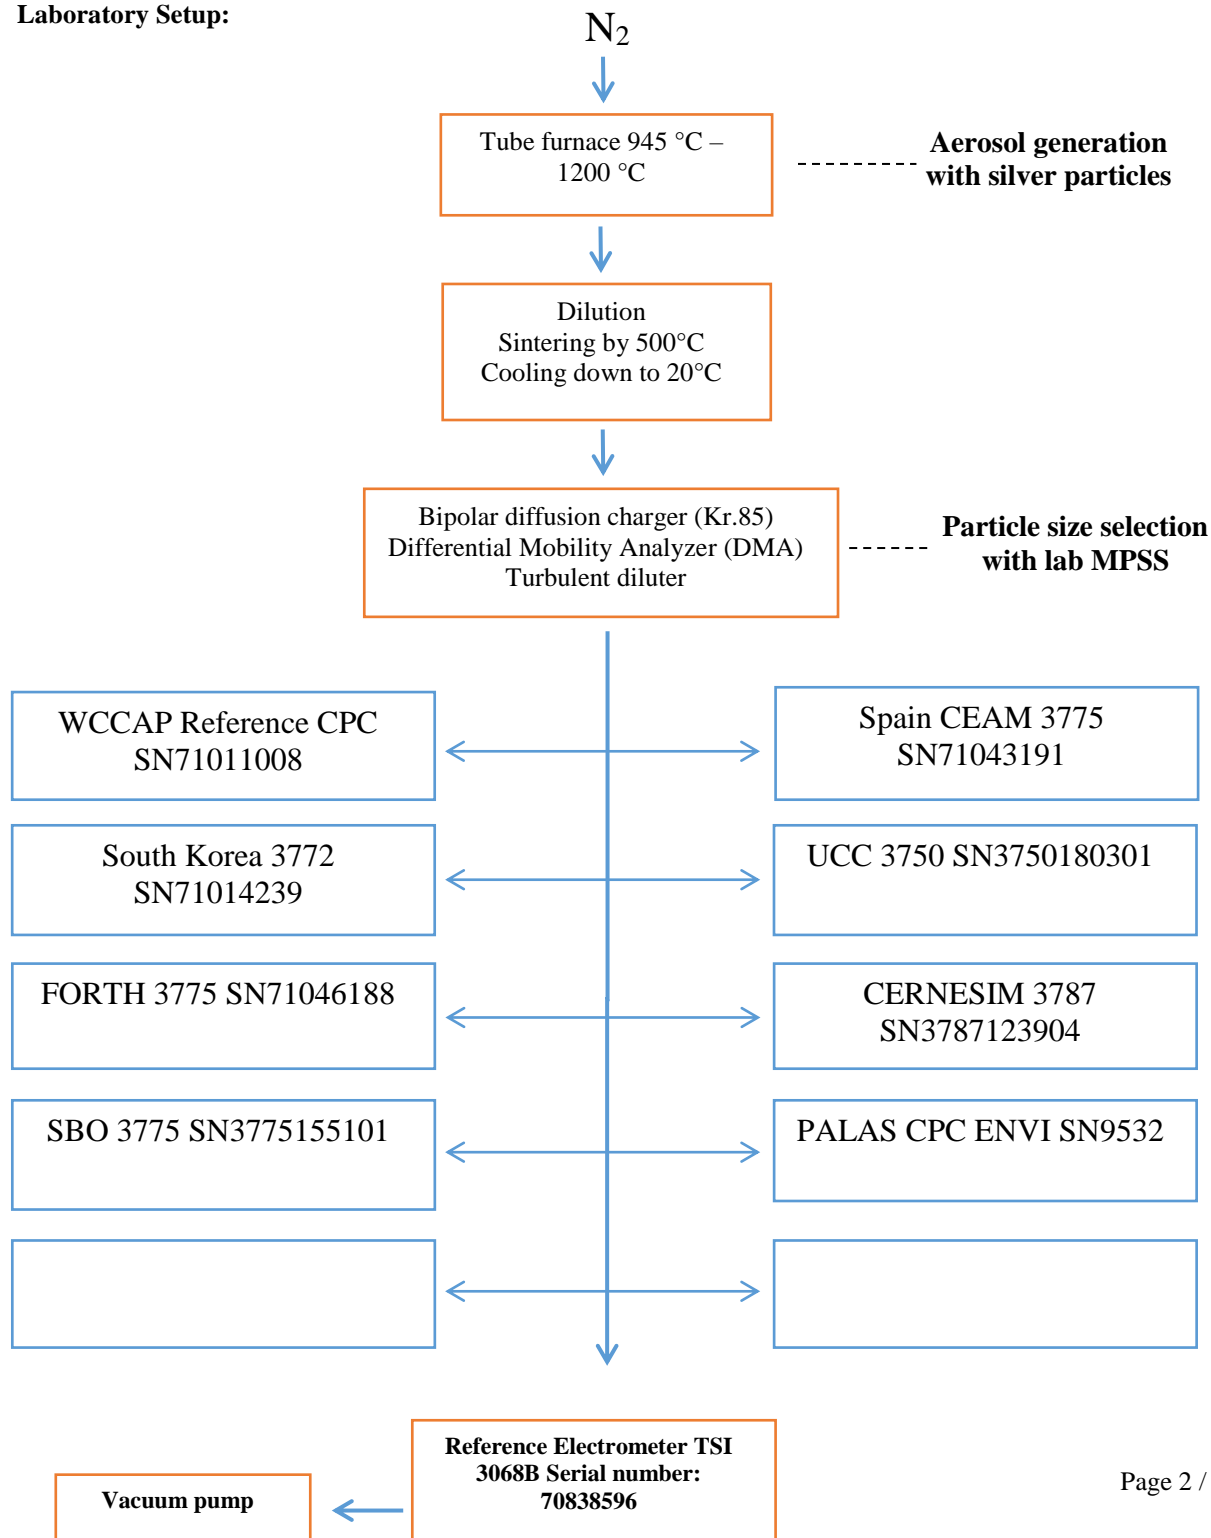



Leibniz Institute for  
Tropospheric Research

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig

**Date of arrival of instrument in calibration lab:**

*October 08, 2019*

**Instrument:**

*Condensation Particle Counter*

**Model and serial number of instrument:**

*CPC 3775 S/N 71046188*

**Result of physical inspection:**

*no damages*

**Result of functional test:**

*no repair*

**Internal parameters of instrument**

*nominal flow rate 0.3 l/min*

**Model and identification number of  
aerosol electrometer:**

*TSI Electrometer Model 3068, S/N 70838596*

**Electrometer calibration certificate:**

*September 05, 2018, calibrated at PTB  
Braunschweig*

**Corrections of electrometer, for instance,  
differing flow rate:**

*Within tolerance range (+/-2%); reference: 4.0  
l/min, measured: 4.00 l/min*

**Software for recording:**

*LabView 2010; National Instruments; Program  
„LabCount.vi“*

**Date of calibration:**

*October 08, 2019*

**Lab temperature and pressure:**

*22.2°C, 985 mbar*

**Measured aerosol flow rate of CPC:**

*0.301(298) l/min*

**Uncertainty in measured flow rate:**

*3%*

**Flowmeter used:**

*Gilian Gilibrator V; S/N 1711008-S,  
January, 2018*

**Particles and gases used for calibration:**

*silver particles and nitrogen*

**Method of particle generation:**

*tube furnace generator*

**Zero measurement of instrument:**

*0 particles/cm<sup>3</sup> in 5 minutes*

**Results (using pulse output):**

Particle size (nm)	40	30	20	15	10
Number concentration (cm-3)	1236	1532	1160	1117	1049
Counting efficiency $\eta$	0.98	0.99	0.97	0.96	0.90
Particle size (nm)	09	08	07	06	05
Number concentration (cm-3)	1260	1791	1545	1483	590
Counting efficiency $\eta$	0.88	0.86	0.82	0.76	0.67
Particle size (nm)	40				
Number concentration (cm-3)	1031				
Counting efficiency $\eta$	0.98				

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig

### Special Information regarding to the Candidate:

Was it necessary to:	yes/no	information
do a second run	no	-
clean the optics	no	-
clean the nozzle	no	-
clean the saturator	no	-
change the wick	no	-
change the laser	no	-
change internal settings	no	-

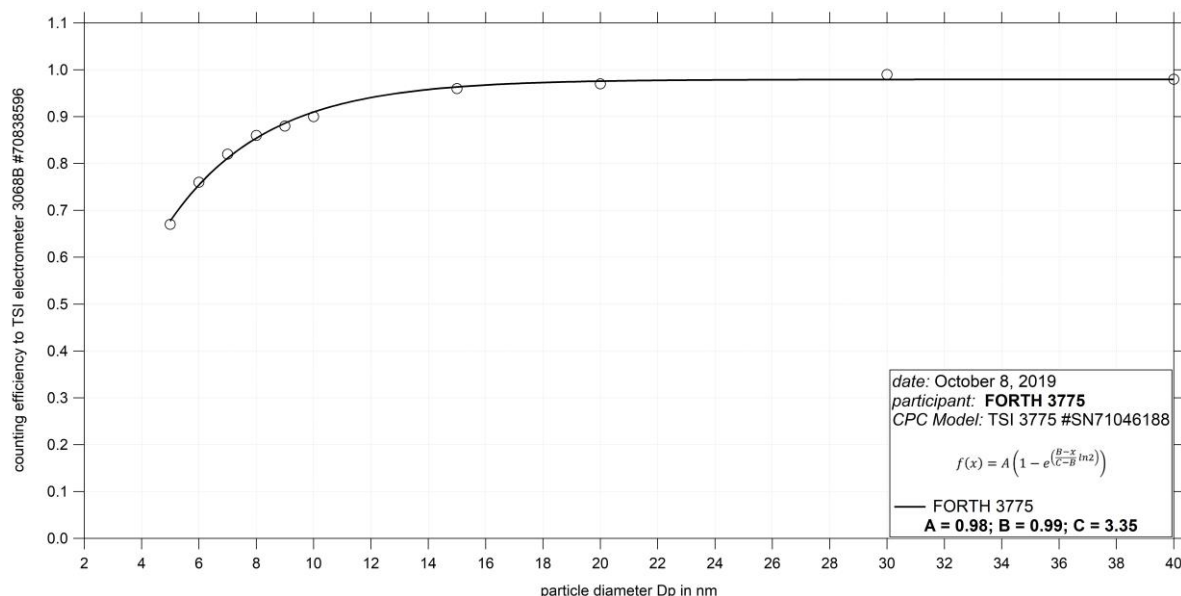


Fig. 1: Counting efficiency for FORTH UCPC 3775 S/N 71046188 against aerosol electrometer 3068 S/N 70838596; silver particles between 5 and 40 nm were used for calibration; the calculated  $Dp_{50}$  is 3.35 nm.

### Status information:

Status	T SAT	T CON	T OPT	T CAB	P AMB
from display	39.0	14.0	40.0	32.7	98.9
Status	P OR	P NO	Laser	LV	flow
from display	87.1	0.054	37mA	full	0.301 (298)

Date of issue: October 08, 2019

Reviewed: TROPOS / Kay Weinhold

Page 4 / 4