

Intercomparison of Condensation Particle Counter

Project No.: CPC-2016-1-5

Basic information:

Location of the quality assurance: TROPOS, lab: 130

Delivery date: -

Setup in the laboratory: January 25, 2016

Comparison period: January 27, 2016

Principal Investigator	Home Institution	Participant	Instrument
Alfred Wiedensohler	Leibniz-Institut für Troposphärenforschung (TROPOS) Permoserstr. 15 04318 Leipzig Germany	-	DE-TROPOS LE-Eiba TSI CPC Model 3010 # 2339

TROPOS Reference Instrument: Electrometer: TSI model 3068B
70838596

Additional Equipment:

- Bubble flow meter 'Gilibrator', Gilian (Sensidyne)

Summary of Intercomparison:

Pre-status:

The TSI CPC Model 3010 was in good condition.

Final status:

The TSI CPC Model 3010 passed the quality standards of ACTRIS and GAW.

On January 27, 2016, the DE-TROPOS LE-Eiba 3010 #2339 participated in the TROPOS ACTRIS-2 CPC-Workshop.

1. Status of the wick: The wick was clean.
2. Status of the CPC: The CPC was working properly.
3. Final CPC-Workshop: The TSI CPC Model 3010 reached 100% efficiency at 30 nm. The Dp50 is at 10.4 nm. The CPC efficiency curve corresponds to the standard.

final-status: 27.01.2016, Wednesday

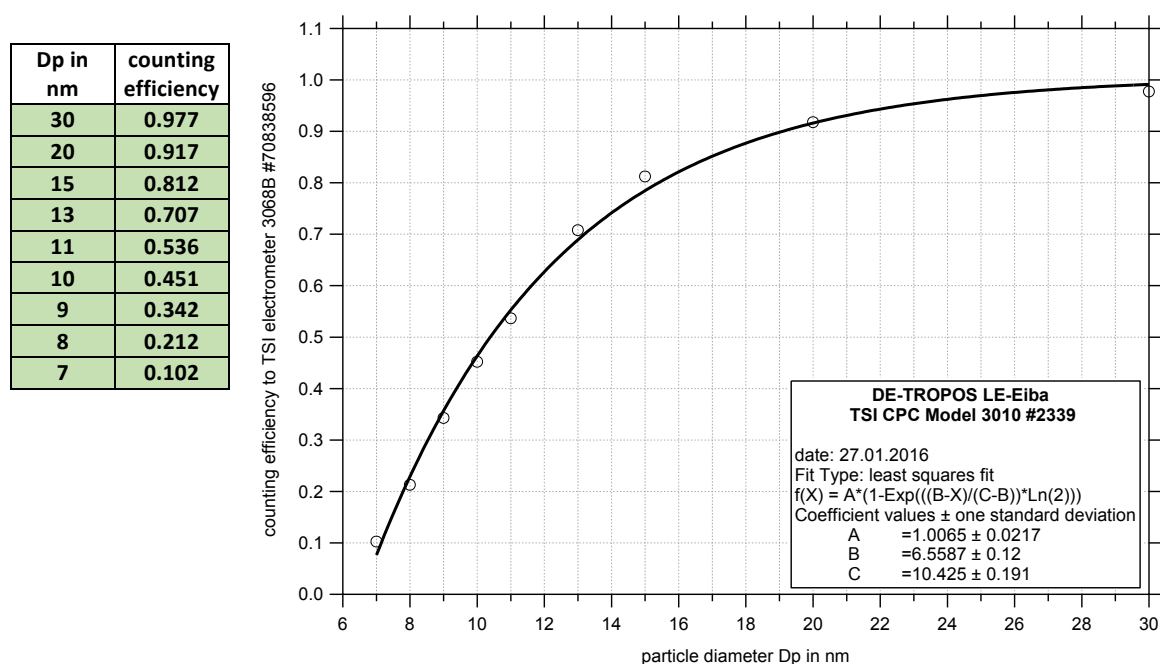


Figure 01: CPC efficiency curve. Based on Electrometer TSI 3068B. Serial number: 70838596