



**World Calibration Centre
for Aerosol Physics**

Leibniz-Institut für Troposphärenforschung Permoserstraße 15 04318 Leipzig



**Leibniz Institute for
Tropospheric Research**

CPC Model: TSI CPC 3750

CPC Serial Number: 3750193807

Customer: TSI Instruments Ltd.

Description: Calibration of a Condensation Particle Counter (CPC, Model 3750)

Date of Calibration: November 13, 2019

Summary of Intercomparison:

The candidate passed the quality standards of ACTRIS and GAW. The candidate reached 98% efficiency at 40 nm. The Dp50 is at 6.90 nm. The CPC efficiency curve corresponds to the standard of ACTRIS and GAW.

Certificate / Reference: WCCAP

Date of issue: November 13, 2019 Signature:

Reviewed by: **TROPOS** Name: **Kay Weinhold**

Page 1 / 4



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

Date of arrival of instrument in calibration lab:

November 11, 2019

Instrument:

Condensation Particle Counter

Model and serial number of instrument:

CPC 3750 S/N 3750193807

Result of physical inspection:

no damages

Result of functional test:

functional test successful, no problems

Internal parameters of instrument

nominal flow rate 1.0 l/min

**Model and identification number of
aerosol electrometer:**

TSI Electrometer Model 3068, S/N 70838596

Electrometer calibration certificate:

*September 5, 2018, calibrated at PTB
Braunschweig*

**Corrections of electrometer, for instance,
differing flow rate:**

*Within tolerance range (+/-2%); reference: 4.0
l/min, measured: 4.000 l/min*

Software for recording:

*LabView 2010; National Instruments; Program
„LabCount.vi“*

Date of calibration:

November 13, 2019

Lab temperature and pressure:

24.5°C, 982.5 mbar

Measured aerosol flow rate of CPC:

1.005 l/min

Uncertainty in measured flow rate:

3%

Flowmeter used:

*Gilian Gilibrator V; S/N 1711008-S,
January, 2018*

Particles and gases used for calibration:

silver particles and nitrogen

Method of particle generation:

tube furnace generator

Zero measurement of instrument:

0 particles/cm³ in 5 minutes

Results (using pulse output):

Particle size (nm)	40	30	20	15	10
Number concentration (cm-3)	1266	1248	1466	1216	1166
Counting efficiency η	0.98	0.98	0.97	0.96	0.81
Particle size (nm)	09	08	07	06	
Number concentration (cm-3)	1230	774	705	443	
Counting efficiency η	0.74	0.64	0.50	0.32	



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

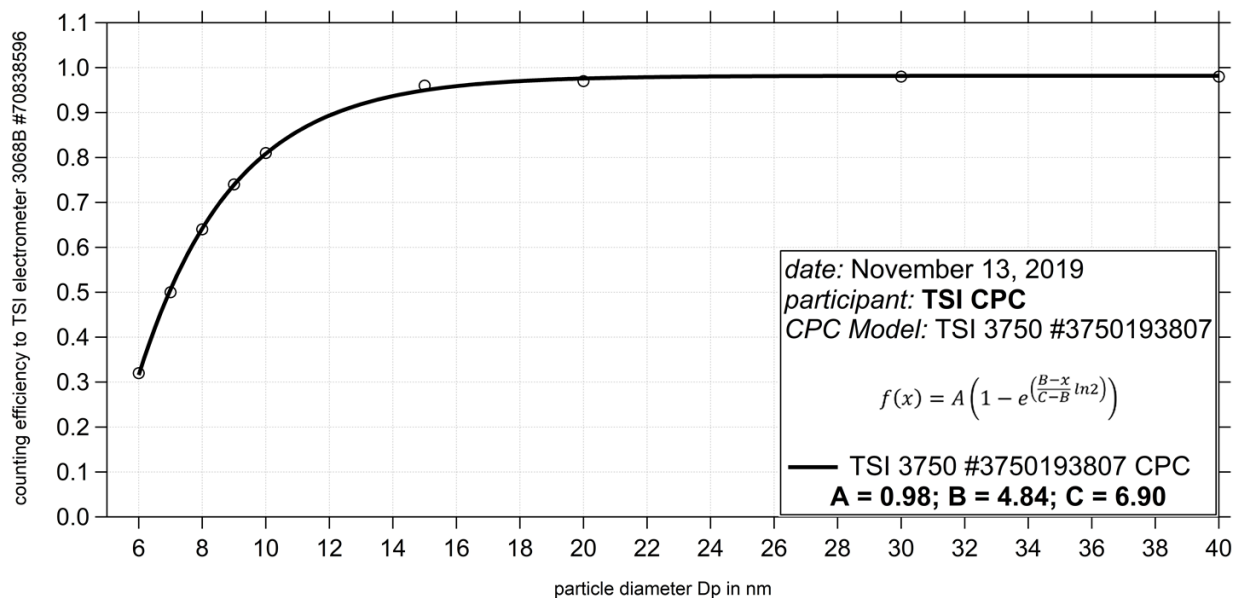


Fig. 1: Counting efficiency for CPC 3750 S/N 3750193807 against aerosol electrometer 3068 S/N 70838596; silver particles between 6 and 40 nm were used for calibration; the calculated Dp50 is 6.90 nm.

Status information:

Status	T SAT	T CON	T OPT	T CAB	P AMB	P VAC
from display	39.0	18.0	40.0	35.4	98.8	82.2
Status	P OR	P NO	Laser	LV	flow	P INLET
from display	80.4	2.41	38	full	1.005	-0.4

Results (using pulse output):

without coincidence correction					
Concentration EM in #/cm ³	66849	58164	50013	43197	32294
Number concentration without coincidence correction (cm-3)	51756	45935	40128	35393	27344
Counting efficiency η	0.77	0.79	0.80	0.82	0.84
Concentration EM in #/cm ³	19887	11244	5127	1177	
Number concentration without coincidence correction (cm-3)	17552	10260	4831	1135	
Counting efficiency η	0.88	0.91	0.94	0.96	



World Calibration Centre
for Aerosol Physics



Leibniz Institute for
Tropospheric Research

with coincidence correction					
Concentration EM in $\#/cm^3$	66849	58164	50013	43197	32294
Number concentration with coincidence correction (cm^{-3})	67872	58316	49325	42408	31437
Counting efficiency η	1.01	1.00	0.98	0.98	0.97
Concentration EM in $\#/cm^3$	19887	11244	5127	1177	
Number concentration with coincidence correction (cm^{-3})	19362	11026	5116	1211	
Counting efficiency η	0.97	0.98	0.99	1.02	

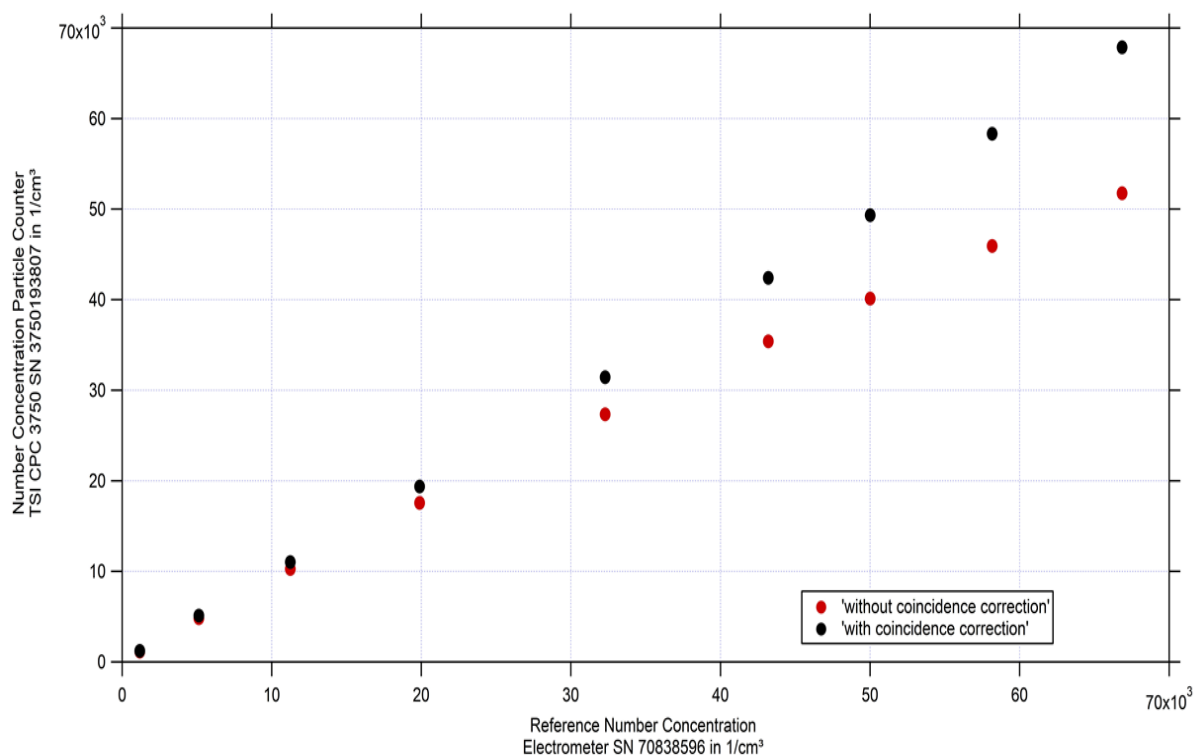


Fig. 2: Linearity test for TSI CPC 3750 SN 3750193807 against aerosol electrometer 3068 SN 70838596; silver particles with a diameter of 30 nm were used for number concentrations between 1000 and 70000 particles per cm^3 .

Date of issue: November 13, 2019

Reference: TSI electrometer, model 3068, SN 70838596

Reviewed: TROPOS / Kay Weinhold

Page 4 / 4